

T3R Antibunching - Slow Decay

Jump to: [navigation](#), [search](#)

[HowTo \(Experimental\)](#); [SymPhoTime](#); [How to perform Hanbury Brown Twiss Antibunching experiments](#); [Diamond NV centers](#) ; [MicroTime 200](#); [Microtime Specials](#); [Antibunching Measurements](#); [Polarisation resolved measurements with the MT200 \(for internal use only\)](#); [total correlation](#)

Q.: How can we avoid decay at very long time delay (up to 5us)?

In this show-case the external preconditions are:

- detectors: perkin elmer SPCMAQR14
- 700 nm SP filter in front of one of the apds
- sample: diamond nanocrystals (100 nm), we are measuring the antibunching of the NV centers emission
- laser wavelength: 532 nm, cw
- T3R Measurement with PicoHarp Software

A.: The decay can be caused by blinking of the nanodiamonds.

A decay caused by correlation statistics

On top of an eventual blinking you will have a decay caused by correlation statistics.

This happens because you correlate the first arriving photon against a photon at the longer time,

which will be an increasingly unlikely event because the earliest stop photons always win and the experiment restarts.

I attached a simulation.

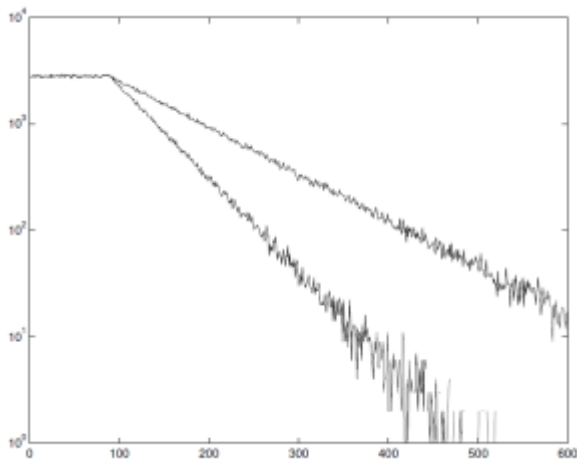


Fig. 1: Logfile logf.png

==== You will need the raw data ==== The timescale is in ns. The plateau is the dead-time. The decay slope depends on the count rate. You can zoom into your data and you will see roughly the same behavior - linear decay after the dead-time, which then of course is overshadowed by the background. The way to avoid this is to calculate the total correlation. This is not a start-stop correlation but the correlation of every photon against every photon. It can be done measuring in T2 mode and then correlating using the SymPhoTime Software (http://www.picoquant.com/products/sw_mt/sw_mt.htm). For a trial you will need the raw data - a pt2 file containing all the photon data - not just the correlated curve. You can record this using the button I highlighted in the attached screenshot.

Copyright of this document belongs to PicoQuant GmbH. No parts of it may be reproduced, translated or transferred to third parties without written permission of PicoQuant GmbH. All information given here is reliable to our best knowledge. However, no responsibility is assumed for possible inaccuracies or omissions. Specifications and external appearances are subject to change without notice.



PicoQuant GmbH
Rudower Chaussee 29 (IGZ)
12489 Berlin
Germany

P +49-(0)30-1208820-89
F +49-(0)30-1208820-90
info@picoquant.com
www.picoquant.com